

Driftline RU validation studies

SUMMARY

AGNAR STEINARSSON



Contents

Foreword..... 2

CPET testing and exercise thresholds..... 2

The IAK study (RU 2019)..... 4

The Runmaker Masters study (RU 2021) 6

The Run and recovery BSc study (RU 2022) 7

The Elderly Fitness Masters study (RU 2024) 9

References..... 11

Foreword

This report briefly summarizes several studies performed at Reykjavik University (RU) in recent years in order to validate Driftline analytics, as patented by Driftline (Steinarsson & Agnarsson, 2020).

- The IAK study (RU 2019)
- The Runmaker Masters study (RU 2021)
- The Run and recovery BSc study (RU 2022)
- The Elderly Fitness Masters study (RU 2024)

The report also contains an opening section about cardiopulmonary exercise testing and exercise thresholds.

CPET testing and exercise thresholds

Cardiopulmonary exercise testing (CPET) is the determination of a person's performance during physical exercise by measuring the metabolic gas exchange. The aim of a standard CPET protocol is to expose the individual to an incrementally increasing workload for about 8 - 12 minutes (incremental ramp protocol) to a volitional maximum. During the test, the patient is connected via mask giving minute ventilation, breathing frequency, oxygen uptake, carbon dioxide production, exercise thresholds and endurance capacity, as well as other parameters.

An important aspect of CPET is the determination of ventilatory exercise thresholds, usually displayed as break points in the CPET graphical displays. Two, and sometimes three, ventilatory thresholds (VT1, VT2 and VT3) can be detected through standard CPET testing. In sports science, however, blood lactate using step protocols is often used for threshold determination. A multitude of threshold concepts exists in the literature, such as Lactate thresholds (LT1, LT2), the Anaerobic threshold (AT), the Respiratory compensation point (RPC) or the Maximal Lactate Steady State (MLSS) (Poole et al., 2021).

Unfortunately, ambiguous threshold terms exist in the scientific literature which can lead to confusion, misunderstanding or even an incorrect interpretation (Binder, 2008). In 2012, a major CPET working group (Westhoff, 2013) decided to refer to the LT and MLSS thresholds as VT1 and VT2, respectively, to avoid this confusion in the future. These terms seem to have gained international acceptance and are now widely implemented in CPET software. Figure 1 shows a simple comparison between *ventilatory and lactate thresholds*.

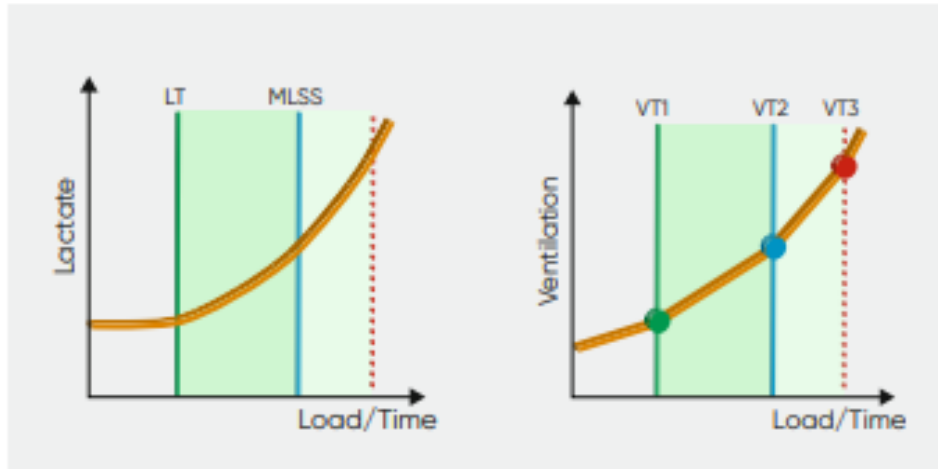


Figure 1. The connection between lactate and ventilatory thresholds (from Vyaire Medical brochure).

The first graph in figure 1 show that the lactate curve is usually exponential in nature with no clear break points and thus, neither the second nor the third (if reached) ventilatory break points can be recognized directly in the lactate curve. Usually the MLSS (often called LT2) is defined as the intensity where blood lactate exceeds 4 mMol/L. As mentioned above, the VT1 and VT2 thresholds correspond to the LT and MLSS thresholds, provided that the measurements were performed under identical conditions. The mandatory interruptions while collecting blood samples for lactate measurements may unduly increase the lactate production and thus interfere with the threshold determination (Vyaire Medical, 2019).

The IAK study (RU 2019)


Co-operation: Driftline, Keilir Sports Academy (IAK), Reykjavík University (RU).

Aim: Validation of Runmaker fitness analytics.

Time of testing: April 2019.

Methods: Eight students performed submaximal treadmill running tests. Four of the students performed cardiopulmonary exercise tests (CPET) at the RU sports laboratory. Measured parameters; VO₂, VCO₂, VO₂max, VE, RER, HR, LT and vVO₂max. Protocol: 2-min step protocol, 1 kph increment, 1% incline/1% increment after 16 kph.

CPET test supervision: Ingi Þór Einarsson professor, Eyþór Oddsson, RU Masters student.

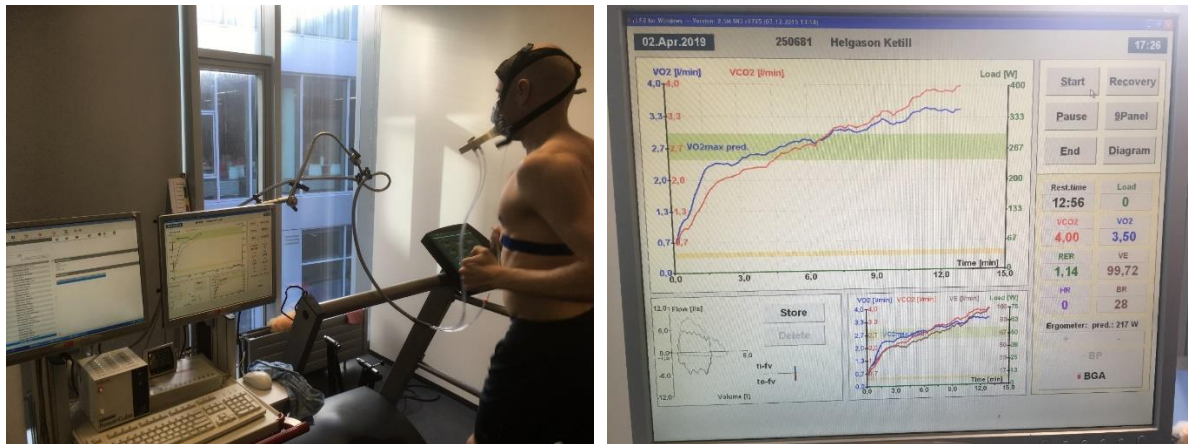

CPET test in the IAK study (April 2nd, 2019).

Example CPET measurements:

Time	Speed	VO ₂ (l/min)	VO ₂ (ml/kg/min)	VCO ₂ (l/min)	RER (VCO ₂ /VO ₂)
0:00-2:00	10 kph	1.68	24.73 (44.02%)	1.33	0.80
2:00-4:00	11 kph	2.44	35.93 (63.96%)	2.17	0.89
4:00-6:00	12 kph	2.74	40.31 (71.75%)	2.58	0.94
6:00-8:00	13 kph	2.96	43.56 (77.55%)	2.98	1.01
8:00-10:00	14 kph	3.17	46.58 (82.92%)	3.32	1.05
10:00-12:00	15 kph	3.43	50.49 (89.88%)	3.77	1.10
12:00-14:00	16 kph	3.56	52.29 (93.08%)	4.07	1.15
14:00-16:00	16 kph 2%	3.71	54.53 (97.08%)	4.60	1.24


VO₂max: 56.2 ml/kg/min

vVO₂max: 16.4 kph

VT-2: 12.8 kph

Results.

Driftline vs CPET validation:

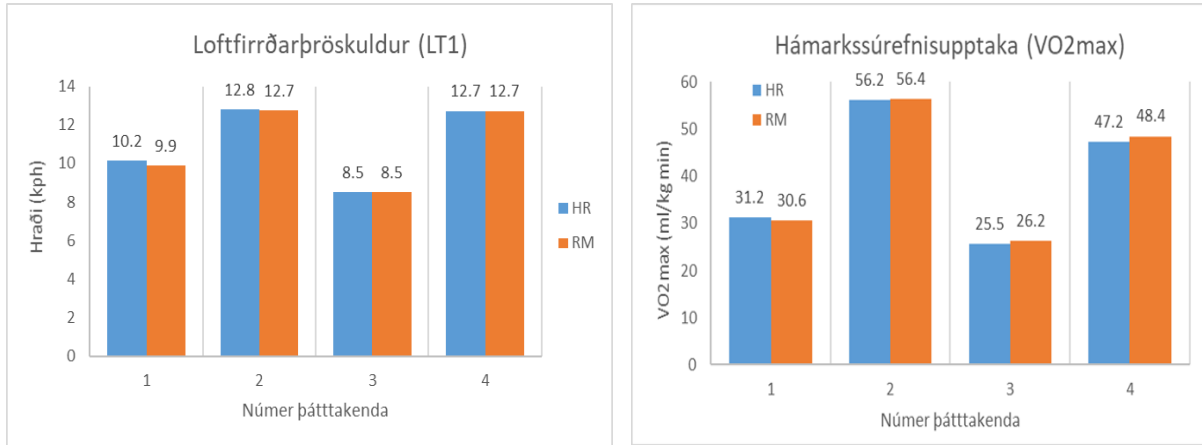

Driftline vs CPET validation. Graph 1 shows the agreement for the LT threshold. Graph 2 shows the agreement for VO2max.

The two graphs show the excellent agreement between Driftline (Runmaker) and gold standard CPET testing for both LT and VO2max.

Conclusion.

This was a small pilot study with the aim to provide some initial validation for the Driftline analytics. The Driftline app was called Runmaker at the time.

The main conclusion from this study was that the Driftline submaximal running test was able to accurately estimate fitness parameters with excellent agreement with gold standard CPET testing. These results paved the way for continued validation studies at the RU Sports Science Department.

The Runmaker Masters study (RU 2021)

Title: Validation and reliability of the Runmaker fitness app.

Author: Ingibjörg Þóra Þórarinsdóttir.

Thesis: Thesis of 45 ECTS credits submitted to the Sports Science Department, School of Social Sciences at Reykjavík University in partial fulfillment of the requirements for the degree of Master of Sports Science and Coaching (June 2021).

Main supervisor: Dr. Ingi Þór Einarsson.

Co-supervisor: Dr. Sigurbjörn Árni Arngrímsson.

Examiner: Dr. Elvar Smári Sævarsson.

Abstract.

Introduction: The maximal oxygen uptake test (VO₂max) is considered to be the most accurate test to assess aerobic capacity. It is one of the most commonly used measurements despite being both complex and demanding. Many different submaximal testing protocols have been developed to make it easier to estimate aerobic endurance and VO₂max. The main objective of this single-blinded laboratory setting research was to test the reliability and validation of the Runmaker fitness app.

Method: Participants were 35, between 16-52 years old, and both male (n=21) and female (n=14). They performed various endurance and anaerobic power tests on separate days: VO₂max, 10-meter sprint and a submaximal endurance test. Six participants aged 16-24 years were asked to perform a submaximal test a second time.

Results: The repeated submaximal measurements in the reliability study showed no statistical difference between variables between tests 1 and 2 ($p > 0.05$). The effect size between the same variables was small to medium (ranging 0.02-0.55). The validity study showed a significant correlation between the measured variables and the predicted variables. The strongest correlation was found between the measured and predicted VO₂max ($r=0.675$) and the measured and predicted HRmax ($r=0.709$).

Conclusion: This study shows that The Runmaker fitness testing app can be considered a reliable and valid test to measure physical parameters by measuring heart rate from a submaximal exercise.

Key words: Aerobic endurance, maximal oxygen uptake, submaximal, heart rate, correlation.

The Run and recovery BSc study (RU 2022)

Title: Assessment of fitness parameters with a submaximal treadmill running test.

Author: Þórey Hákonardóttir and Jón Oddur Guðmundsson.

Report: Report submitted to the Sports Science Department, School of Social Sciences at Reykjavík University in partial fulfillment of the requirements for the degree of Bachelor of Sports Science and Coaching (June 2022).

Supervisor: Dr. Ingi Þór Einarsson.

Abstract.





Introduction: Cardiopulmonary exercise testing (CPET) is widely recognized as the gold standard test for measuring aerobic capacity. However, the laboratory-based CPET is very physically demanding and not easily accessible to the general public. The main aim of this single-blind laboratory setting research was to validate the Driftline submaximal assessment of fitness parameters.

Method: Participants were 30, between 21-48 years old, and both male (n=19) and female (n=11). They performed various tests on separate days: walking treadmill test, CPET, 10-meter sprint and a 20-min submaximal endurance test. A lactate blood sample was taken after 15 minutes of the submaximal test with 15-min passive recovery.

Results: The study showed a significant correlation between measured and predicted variables. The strongest correlation was found between the measured and predicted HRmax ($r=0.883$) and the measured and predicted VO₂max ($r=0.737$). The average, measured and predicted VO₂max values were 51.2 ± 10.4 and 52.6 ± 9.7 ml/kg/min, respectively. The average, measured and predicted HRmax values were 184.1 ± 8.4 and 188.3 ± 8.7 bpm, respectively. The average, measured and predicted Vmax values (max sprinting speed) were 26.4 ± 3.1 and 25.9 ± 2.9 bpm, respectively. The average, measured and predicted LT-1 threshold speeds were 9.9 ± 1.8 and 9.9 ± 1.7 km/hour, respectively. The average, measured and predicted LT-2 threshold speeds were 14.3 ± 2.8 and 13.9 ± 2.6 km/hour, respectively.

Figures.

A highly significant correlation was found between measured and predicted fitness parameters, as shown on the graphs on the next page.

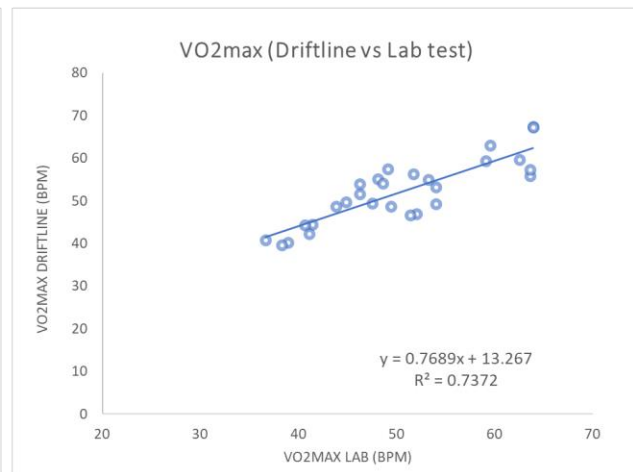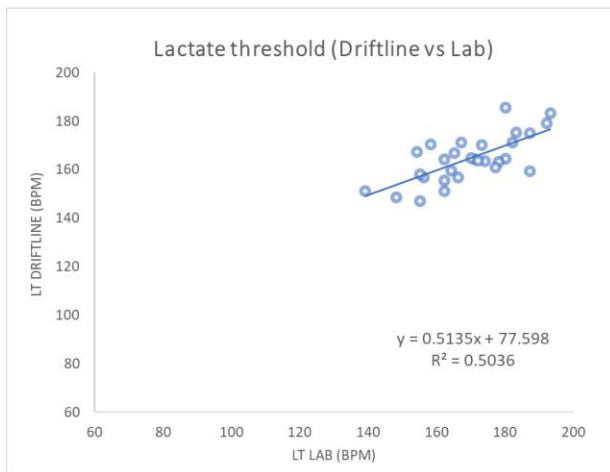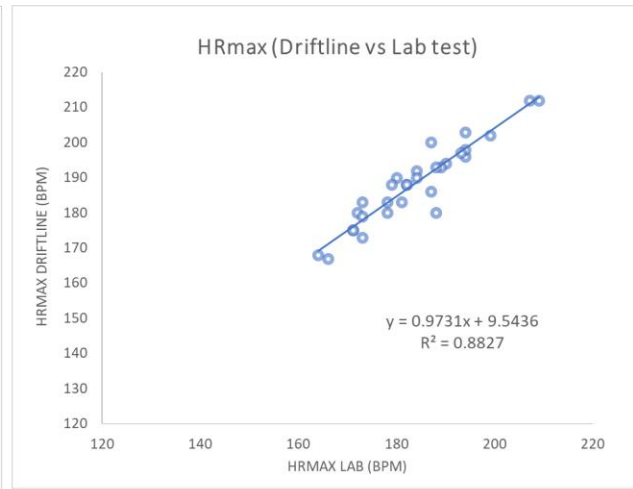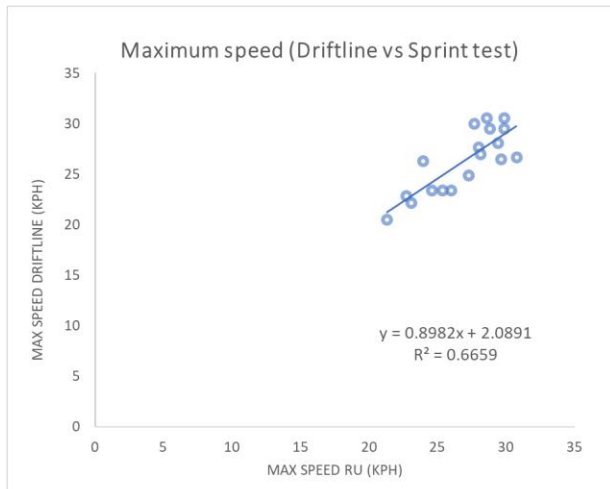

Conclusion: This study shows that Driftline submaximal fitness test can be considered a reliable and valid test to assess fitness parameters from heart rate analysis.

Key words: Aerobic endurance, maximal oxygen uptake, submaximal, heart rate, correlation.

The Elderly Fitness Masters study (RU 2024)

Title: Different sub-maximal tests to evaluate aerobic endurance among older adults.

Author: Þórey Hákonardóttir.

Thesis: Thesis of 45 ECTS credits submitted to the Sports Science Department, School of Social Sciences at Reykjavík University in partial fulfillment of the requirements for the degree of Master of Sports Science and Coaching (June 2024).

Supervisor: Ingi Þór Einarsson.


Key words: Exercise science and coaching, Aging, Health, Exercise.

Abstract

Introduction: Exercise is well-known for improving quality of life and health. As longevity increases, paying attention to well-being becomes more crucial. Driftline is an Icelandic start-up company introducing HR monitoring that measures aerobic endurance from 0-100%.

Objective: If 6- and 12-minute treadmill walking tests are valid and reliable measurements compared to the 6-minute walking test on the floor (6MWT) and if Driftline's analytics can assess aerobic endurance among older adults using sub-maximal testing protocols.


Methods: 42 older adults (60% female, mean age 71.93 ± 4.68) participated in four submaximal endurance tests: 6MWT on the floor, 6MWT on a treadmill, 12MWT on a treadmill, and 6MWT at a self-selected speed on a treadmill. A total of 28 participants completed all tests. Heart rate (bpm) was monitored throughout the tests, with a ten-minute seated rest period after the tests. A repeated measures ANOVA was conducted along with Pearson correlation.

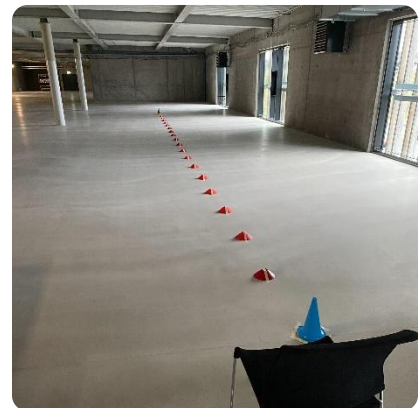

Results: There was a significant correlation between the 6MWD on the floor and the treadmill in all tests ($r=0.955-0.874$). There were significant differences ($p<0.001$) between treadmills and 6MWT on the floor, with an 83.36 ± 31.77 m difference in distance walked, a 14% lower HR response, and a reduced step frequency of $5.46 \pm 0.82-9.37 \pm 0.44$ steps/min. Driftline Analytics' endurance scale significantly correlated with walking distances in all tests ($r=0.350-0.469$).

Six-minute-walking-test (6MWT). Agreement between test and estimation:

Among the parameters calculated by Driftline was the estimated maximum walking speed for each of the participants, based on a novel method of gait analysis. The calculated maximum speed (from a submaximal treadmill test) showed excellent agreement with the measured 6MWT floor distance (6MWD), as shown in the two graphs below:

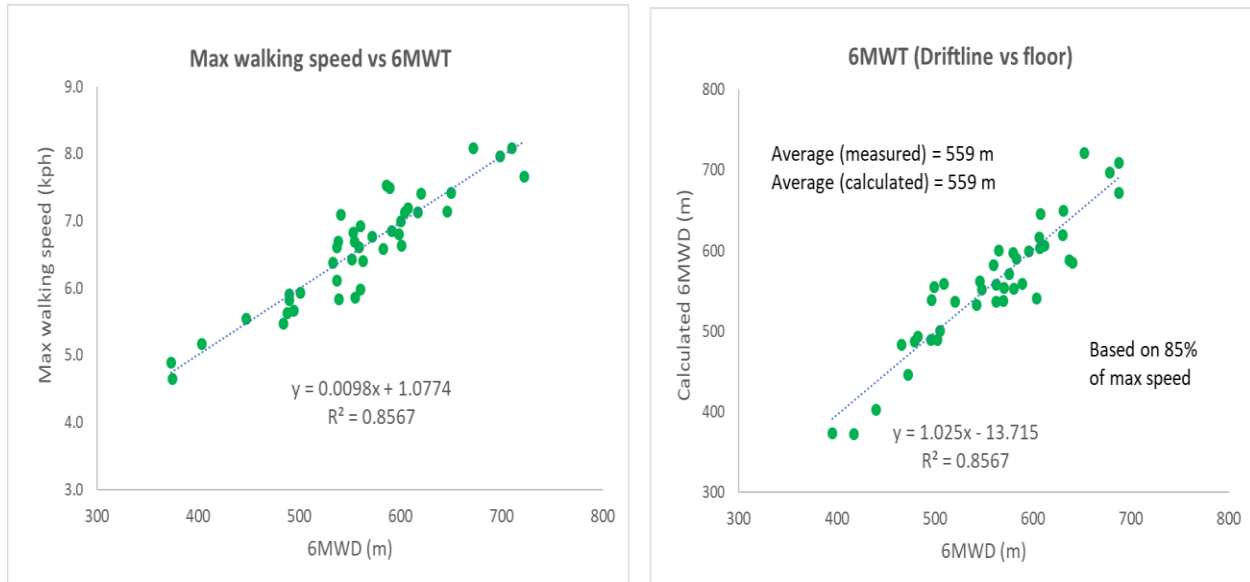

The first graph shows a highly significant correlation between 6MWD and the calculated max walking speed. The second graph shows a highly significant correlation between measured and calculated 6MWD.

Conclusions: The 6MWT and 12MWT on a treadmill are valid alternatives to the 6MWT on the floor for assessing aerobic endurance in older adults, and the U-turns in the 6MWT have an effect. Driftline's heart rate analysis can be used at sub-maximal effort.

The results show that the six-minute walking distance only shows a weak correlation with aerobic endurance, as defined and measured by Driftline, but on the other hand a very strong correlation with the estimated maximum walking speed. Apparently, maximum power and speed are more important for performance than endurance in such a short walking test.

The main conclusion is that with the Driftline analytics it is possible to use a submaximal treadmill walking test to approximate performance in a six-minute walking test with high accuracy.

References

- Binder, R. K., Wonisch, M., Corra, U., Cohen-Solal, A., Vanhees, L., Saner, H., & Schmid, J. P. (2008). Methodological approach to the first and second lactate threshold in incremental cardiopulmonary exercise testing. *European journal of cardiovascular prevention and rehabilitation*, 15(6), 726–734.
<https://doi.org/10.1097/HJR.0b013e328304fed4>
- Ingibjörg Þóra Þórarinsdóttir (2021). Validation and reliability of the Runmaker fitness app. Thesis of 45 ECTS credits submitted to the Sports Science Department at Reykjavík University in partial fulfillment of the requirements for the degree of Master of Sports Science and Coaching (June 2021).
- Poole, D. C., Rossiter, H. B., Brooks, G. A., & Gladden, L. B. (2021). The anaerobic threshold: 50+ years of controversy. *The Journal of physiology*, 599(3), 737–767.
<https://doi.org/10.1113/JP279963>
- Steinarsson, A. & Agnarsson, S. (2020). A method and system for determining exercise parameters including aerobic endurance based on heart rate curve analysis. Patent number 4106624. <https://patents.google.com/patent/WO2021166000A1/en>
- Vyair Medical. (2019). Special Edition Cardiopulmonary Exercise Testing. Eschenbacher, H. (ed). CareFusion Germany 234 GmbH.
https://www.vyair.com/sites/us/files/2019-04/Special-Edition-CPET_EN_Web.pdf
- Westhoff, M., Ruhle, K., Greiwing, A., Schomaker, R.M., Eschenbacher, H., Siepmann, M., & Lehnigk, B. (2013). Ventilatorische und metabolische (Laktat-)Schwellen. *Deutsche Medizinische Wochenschrift*, 138, 275 - 280.
- Þórey Hákonardóttir (2024). Different sub-maximal tests to evaluate aerobic endurance among older adults. Thesis of 45 ECTS credits submitted to the Sports Science Department at Reykjavík University in partial fulfillment of the requirements for the degree of Master of Sports Science and Coaching (June 2024).
<https://hdl.handle.net/1946/47765>